REF Q-NCOV-01G

STANDARD O COVID-19 A

STANDARD™ Q COVID-19 Ag Test PLEASE READ CAREFULLY BEFORE YOU PERFORM THE TEST

SD BIOSENSOR

* It is recommended to perfrom ANTIGEN TEST WITHIN 6 DAYS after symptom onset, and ANTIBODY TEST FROM 7 DAYS after symptom onset.

COVID-19 Ag Test Test device (individually in Nozzle cap Paper stand

PREPARATION

Carefully read instructions for using the STANDARD Q COVID-19 Ag Test.



2 Check the expiry date at the back of the foil pouch. Do not use the kit, if expiry date has passed.



3 Check the test device and the desiccant pack in the foil pouch.

buffer tube

KIT CONTENTS

a foil pouch with desiccant)



TEST PROCEDURE


1 Insert a sterile swab into the nostril of the patient, reaching the surface of the posterior nasopharynx.



2 Swab over the surface of the posterior nasopharynx.




3 Withdraw the sterile swab from the nasal





4 Insert the swab into an extraction buffer tube. While squeezing the buffer tube, stir the swab more than 5 times.

use



5 Remove the swab while squeezing the sides of the tube to extract the liquid from the swab.


















• Do not read test results after 30 minutes. It may give false results.

INTERPRETATION OF TEST RESULT

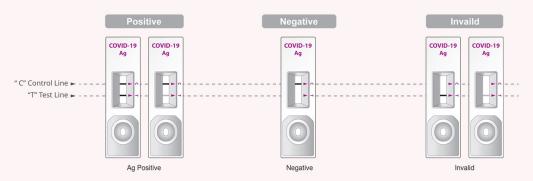

- 1. A colored band will appear in the top section of the result window to show that the test is working properly. This band is control line (C).
- 2. A colored band will appear in the lower section of the result window. This band is test line of SARS-CoV-2 antigen (T).
- 3. Even if the control line is faint, or the test line isn't uniform, the test should be considered to be performed properly and the test result should be interpreted as a positive result.

 * The presence of any line no matter how faint the result is considered positive.
- * Positive results should be considered in conjunction with the clinical history and other data available.